



Tech Works Guide to Proposed 2026 FGI Nurse Call Function Locations in Outpatient Facilities

		Station type required:	DOME LIGHT	DOME LIGHT	Patient	Staff Assist	Emergency Call	Toilet Room Call
		Station Definitions			A device that a patient can reach from a bed or exam table or chair	A device to indicate the need for staff assistance	A device to indicate emergency assistance is needed (i.e., code blue signal)	A device with a pull cord that hangs to a length of 6 inches above the finished floor
		Tech Works Station Part Number:	NC-DL-12-R	NC-DL-22-BR	NC-PBS-1 W/PBC-7	NC-SAS unless replaced by NC-PBS-1 or NC-CBAS	NC-CBS or NC-CBAS	NC-EPS
		Device						
		Symbol						
Section	Locations:	Location Definition						
Recommended								
2.1-3.2.2	Exam Rooms	A room designated for the performance of patient care activities that may require high-level disin-fected or sterile instruments but do not require the envi-ronmental controls of a procedure room.	X			X		
2.1-3.2.2.2	Single-patient exam/observation room	A room designated for the performance of patient care activities that may require high-level disin-fected or sterile instruments but do not require the envi-ronmental controls of a procedure room.	X			X		
2.1-3.10.2	Patient Toilet Room	Patient toilet rooms shall be separate from public use toilet rooms and located to permit access from patient care areas without passing through publicly accessible areas. Patient toilet rooms shall be equipped with a toilet(s) and a handwashing station	X					X
Required								
2.1-3.2.3	Procedure room (including endoscopy)	A room designated for the performance of patient care activities that may require high-level dis-infected or sterile instruments and some environmental controls but do not require the environmental controls of an operating room.		X		X	X	
2.3-3.2.3	Class 2 imaging room	An imaging room designated for the performance of patient care activities that may require high-level disinfected or sterile instruments and some en-vironmental controls but do not require the environmen-tal controls of a Class 3 imaging room.		X		X	X	
2.1-3.2.4	Operating room	A room within the surgical suite that is designated and equipped for performing surgical or other invasive procedures, meeting the requirements of a restricted area, and requiring an aseptic field for all procedures performed within it.		X		X	X	
2.3-3.2.4	Class 3 imaging room	An imaging room that meets the definition of an operating room and has equipment to enable diagnostic imaging before, during, and after surgi-cal procedures.		X		X	X	
2.1-3.7.3	Pre-procedure patient care station	A designated space for the perfor-mance of a specific patient care function for one patient at a time.		X	X	X	X	
2.1-3.7.4	Phase I post-anesthesia recovery (PACU) patient care station	A POST-ANESTHESIA CARE UNIT (PACU) patient care station is required for each operating room		X	X	X	X	
2.1-3.7.5	Phase II recovery patient care station	A minimum of one patient care station per imaging, procedure, or operating room		X	X	X	X	
2.8-3.4.2	Emergency facility treatment room	A standard patient room in an emergency department (ED) or urgent care center that can be used for a variety of functions, including Patient examination, Treatments Procedures, such as wound packing, suture placement, or casting		X	X	X		
2.8-3.4.8.2	Low-acuity patient treatment station	An area in an emergency de-partment or facility where patients with less urgent needs can be treated in bays or cubicles sized to accommodate a patient chair.		X	X			
2.8-3.4.9.2	Human decontamination room	A facility where people who are suspected of being contaminated are cleaned and provided with new clothing. Decontamination is the process of removing or neutralizing hazardous substances from people, equipment, and the environment. The outside entry door for the decontamination area should be at least 10 feet from the closest other entrance. It should also be at least 30 feet from ambulance entrances		X			X	
2.8-6.2.2	Emergency facility triage area	A dedicated space within an emergency department where patients are initially assessed upon arrival to determine the severity of their condition and prioritize their need for immediate medical attention		X	X	X		
2.10-3.2.2	Hemodialysis patient care station	A dedicated area within a dialysis center where a patient receives their hemodialysis treatment		X	X		X	
2.10-3.3	Dialysis facility home training room	Where patients are trained to use dialysis equipment at home, a private room of at least 120 square feet		X	X		X	
2.10-3.10.2	Dialysis facility patient toilet	A dedicated toilet within a dialysis center that is specifically designed for use by patients undergoing dialysis treatment	X					X
2.11-3.10.2.2 (2)	Electroconvulsive therapy (ECT) room	ECT is a medical procedure that involves passing a small electric current through the brain to trigger a seizure. It's a treatment for severe depression and other mood disorders and is performed under general anesthesia		X		X	X	
2.11-3.10.2.2 (3)	ECT recovery patient care station	A recovery patient care station as part of the requirements for Electroconvulsive Therapy (ECT) treatment and recovery		X		X	X	
2.11-3.2.2	Behavioral health exam room	A space within a Behavioral health facility for patient care activities that may require sterile or disinfected instruments, but do not require the environmental controls of a procedure room		X		X	X	
2.12-3.2	Behavioral health crisis center exam room	A space within a Behavioral health crisis center for patient care activities that may require sterile or disinfected instruments, but do not require the environmental controls of a procedure room		X		X	X	
2.12-3.9	Group room for community- based crisis center	An open room for multiple individuals, known as a "milieu," where patients are free to move about, helping reduce anxiety		X		X	X	
2.12-4.1	Behavioral health crisis center nurse station	A multipurpose staff work area used by all caretakers in a patient care or diagnostic area.		X		X	X	


Tech Works is not affiliated with FGI in any way.
These recommendations are Tech Works opinion based on our experience.
In all cases consult Authorities Having Jurisdiction (AHJ) for compliance to local building codes.
Tech Works will not be held liable for any building code compliance.
All products shown are UL1069 compliant for use in Outpatient Medical Clinics.

PLAN LAYOUT EXAMPLES


Single-patient exam/ observation room

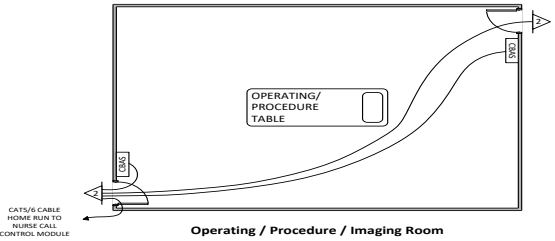

Pre-procedure patient care station / Post Op PACU / Phase II recovery / Emergency facility treatment room

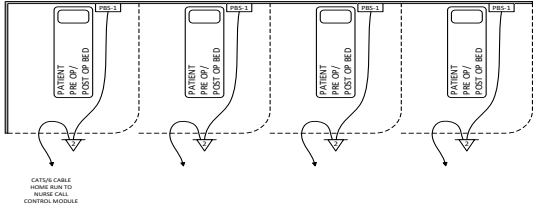

Hemodialysis patient care stations

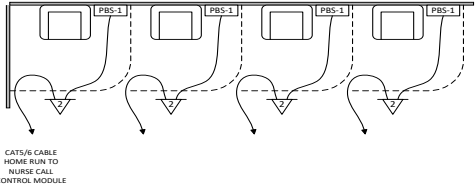

Patient Toilet

